

Instructions for Use (Handbook)

MagPurix[®] Viral Nucleic Acid Extraction Kit

Catalog No.: ZP02003
Manual No.: IFU-MP02-02003
Version: 2.2



For *in vitro* diagnostic use



Obelis s.a.
Bd Général Wahis 53
1030 Brussels Belgium
Tel: +(32) 2 732-59-54
Fax: +(32) 2 732-60-03
mail@obelis.net



ZINEXTS LIFE SCIENCE CORP.
16F., No. 93, Sec. 1, Xintai 5th Rd.,
Xizhi Dist., New Taipei City 221416,
Taiwan (R.O.C.)

Read and follow these Instructions for Use prior to using this product. The latest revision of this document can be found at www.zinexts.com

Contents

Intended Use	3
Introduction	3
Kit Contents and Storage.....	3
Materials Required But Not Provided	4
Warnings and Precautions	5
Purification Principle.....	6
Things to Do Before Starting	7
Sample Preparation	7
Preparation of RNA Carrier	8
 Procedure of MagPurix System	9
Purification Protocol - MagPurix® series	9
Purification Protocol - MagPurix® EVO series	10
Troubleshooting	11
Related Products.....	12
References	13
Symbols.....	13
Limited Product Warranty.....	14
Revision History	14

Intended Use

The MagPurix® Viral Nucleic Acid Extraction Kit contains all required reagents and consumables for the rapid automated purification of viral DNA and RNA from serum, plasma, cell-free body fluids, and clinical swab samples in transport medium, using the MagPurix system.

The product is intended to be used by professional users, such as technicians and physicians who are trained in molecular biology techniques.

Introduction

Product Name	MagPurix® Viral Nucleic Acid Extraction Kit
Catalogue Number	ZP02003
Product Overview	The MagPurix® Viral Nucleic Acid Extraction Kit is designed to extract viral nucleic acid from serum, plasma, cell-free body fluids, and clinical swab samples in transport medium using MagPurix® series automated instruments. The unique magnetic ZiBeads® technology enables purification of high-quality nucleic acids that are free of proteins, nucleases, and other impurities. The final product is suitable for a wide range of diagnostic and research applications, such as sequencing, genotyping, PCR, RT-PCR, and NGS assays.
Applicable Instrument Model	All MagPurix® Instruments
Display Protocol Name on The Instrument	2003 VIRAL 2003 VIRAL RAPID (EVO only)
Applicable Instrument Firmware	Check and download the latest firmware from www.zinexts.com
Processing Time	MagPurix® 12 series 40-55 minutes MagPurix® 24 series 40-70 minutes MagPurix® EVO series 40-50 minutes (RAPID : 19-23 min)

Kit Contents and Storage


Shipping and Storage	The kit is shipped at room temperature. Upon receipt, store the kit at room temperature. All kit components are stable when stored properly until the expiration date shown on the kit box.	
Kit Content	The components supplied in the kit are listed below. Sufficient reagents are supplied to perform 48 purifications.	
	Contents	Amount
	1 Reagent Cartridge	48 pcs (6x8)
	2 Reaction Chamber	48 pcs (6x8)
	3 Tip Holder	48 pcs (6x8)
	4 Piercing Pin	50 pcs

5 Filter Tip	50 pcs
6 Sample Tube (2 ml)	50 pcs
7 Elution Tube (1.5 ml)	50 pcs
RNA Carrier (1 mg)	1 pc
Barcode Sticker (EVO only)	50 pcs

Reagent
Cartridge
Contents

Each Reagent Cartridge has 10 positions with 10 sealed well. Positions 1-10 contain wells filled reagents for this protocol.

Reagent	Well No.
Proteinase K Solution	1
Lysis Buffer 4	2
Binding Buffer 1	3
Magnetic Bead Solution	4
Washing Buffer 2	5
Washing Buffer A	6
Washing Buffer B	7
RNase-free water	8
RNase-free water	9
Empty	10

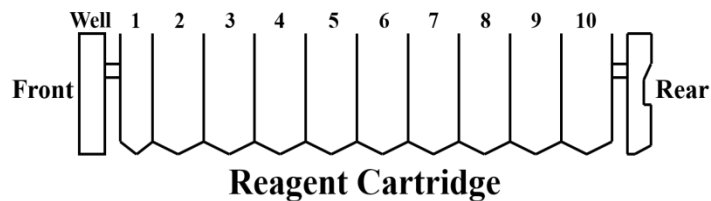

Materials Required But Not Provided

The following general laboratory equipment and consumables are required to perform the extraction. All laboratory equipment should be installed, calibrated, operated, and maintained according to the manufacturer's recommendations. The following table lists the required equipment and consumables.

For all purification procedures:
1. MagPurix® / MagPurix® EVO series instrument
2. 1.5 or 2.0 ml microcentrifuge tubes
3. Pipettes and filter tips
4. Phosphate-buffered saline (PBS, may be required for diluting samples)
5. Optional: Plastic consumables, DNase-free RNase A (to minimize RNA content)

Warnings and Precautions

For *in vitro* diagnostic use only. Read all the instructions carefully before using the kit. Use of this product should be limited to trained personnel in the techniques of DNA purification. Strict compliance with the user manual is required for optimal results. Attention should be paid to expiration dates printed on the box and labels of all components. Do not use a kit after its expiration date.


When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, please consult the appropriate safety data sheets (SDSs). These are available online in convenient and compact PDF format at **MSDS (Material Safety Data Sheets) – Downloads – www.zinexts.com**.

Please report any serious incident occurred in relation to the device to your local representative/agent or the manufacturer, and to the competent authority of your country/state.



CAUTION: DO NOT add bleach or acidic solutions directly to the sample preparation waste.

Purification Principle

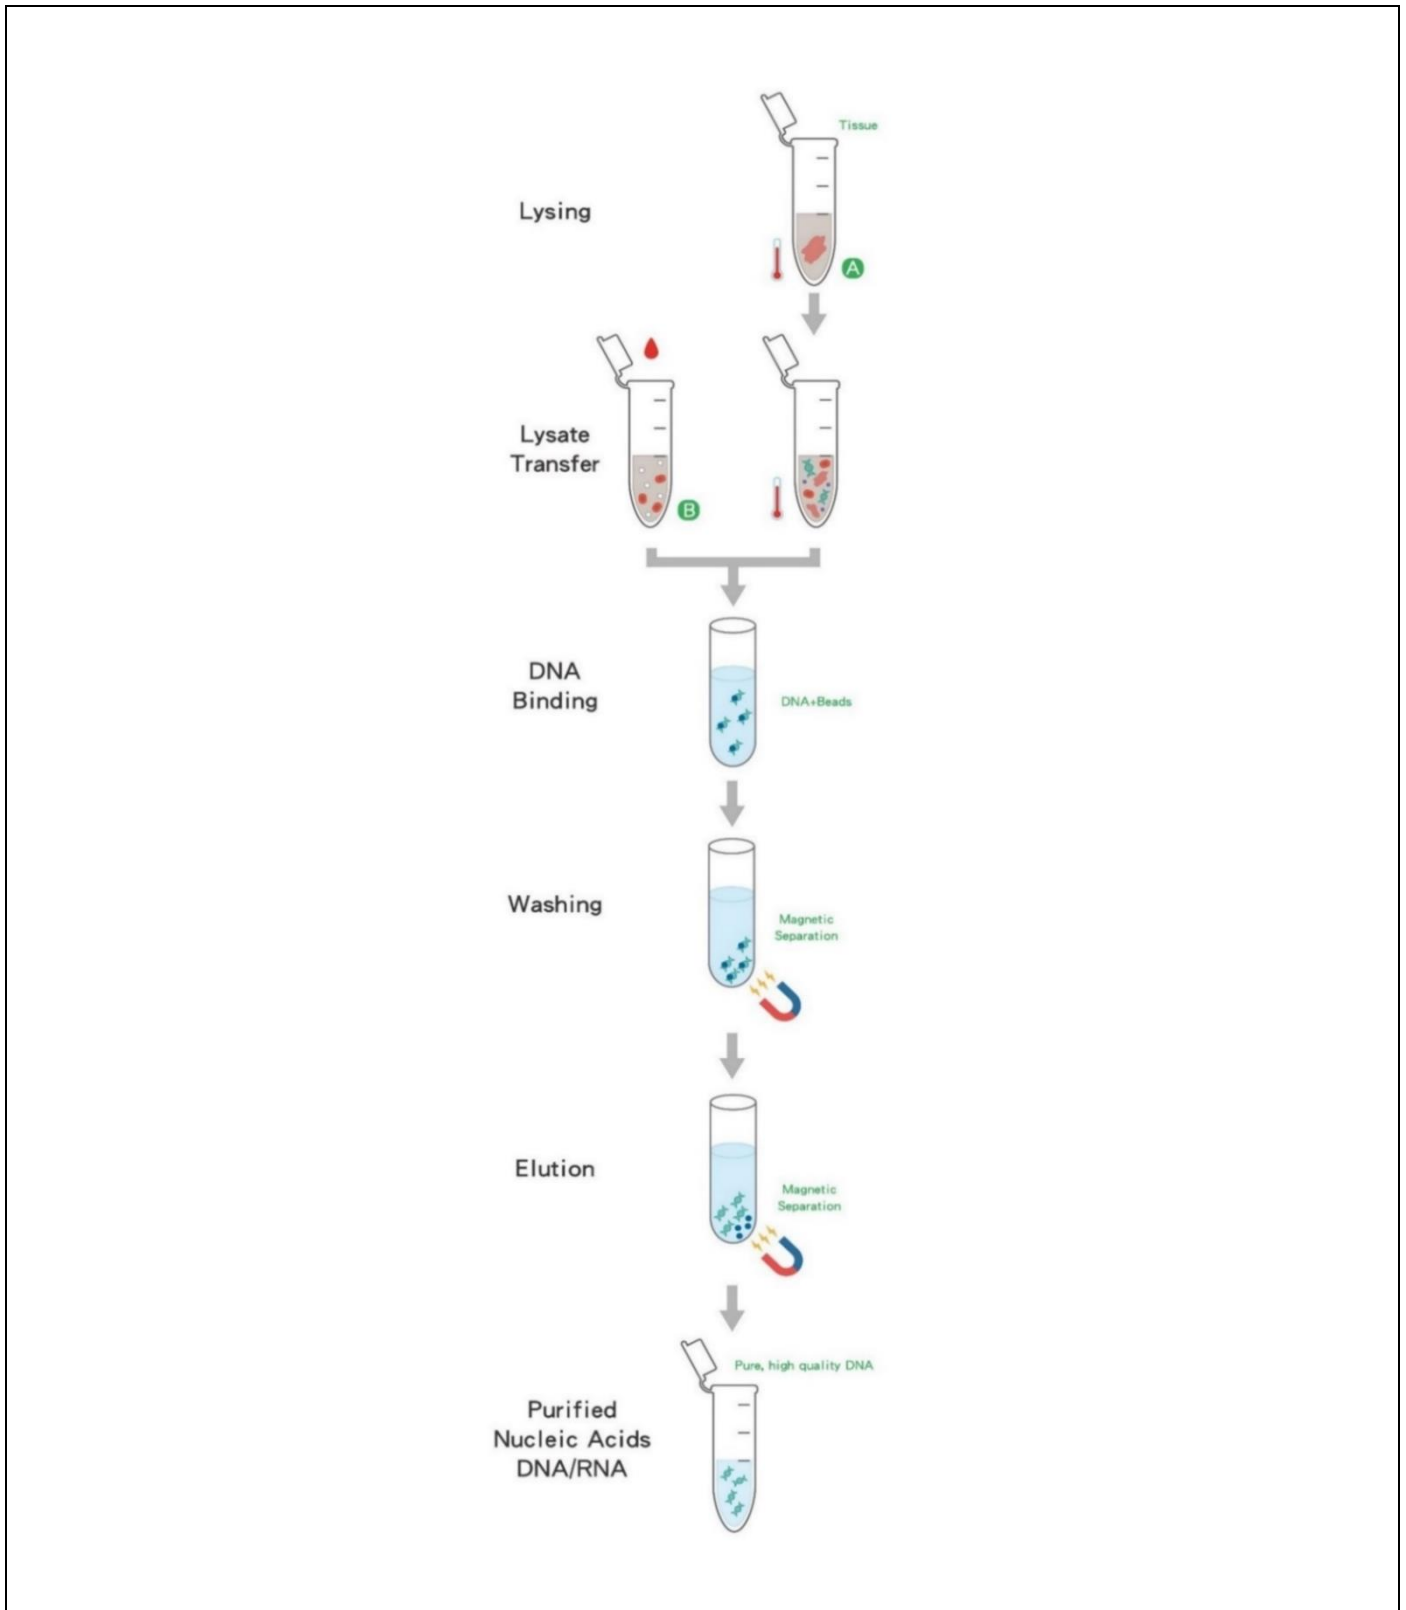

- A** Perform certain pretreatment process before extraction.
- B** Transfer sample to extraction directly.

Things to Do Before Starting

Sample Preparation

The purification procedure is optimized for the use of 100-560 μ l (EVO 100-400 μ l) serum, plasma*, CSF, pretreated urine, cell-free body fluid samples or clinical swab samples.

Serum	<ol style="list-style-type: none"> Add an appropriate volume of RNA Carrier into each Sample Tube. Dispense 100-560 μl (EVO 100-400 μl) of sample into each Sample Tube. If the sample volume is lower than described, please complete the volume with appropriate amount of 1X PBS.
Plasma	<ol style="list-style-type: none"> Add an appropriate volume of RNA Carrier into each Sample Tube. Dispense 100-560 μl (EVO 100-400 μl) of sample into each Sample Tube. If the sample volume is lower than described, please complete the volume with appropriate amount of 1X PBS.
Cerebrospinal fluid (CSF)	<ol style="list-style-type: none"> Add an appropriate volume of RNA Carrier into each Sample Tube. Dispense 100-560 μl (EVO 100-400 μl) of sample into each Sample Tube. If the sample volume is lower than described, please complete the volume with appropriate amount of 1X PBS.
Urine	<ol style="list-style-type: none"> Centrifuge the sample at 20,000 x g for 10 minutes to concentrate the virus into a pellet. Discard supernatant and resuspend the pellet in 220 μl of 1X PBS. Transfer 200 μl concentrated sample into each Sample Tube.
Cell-free body fluid(s)	<ol style="list-style-type: none"> Add an appropriate volume of RNA Carrier into each Sample Tube. Dispense 100-560 μl (EVO 100-400 μl) of sample into each Sample Tube. If the sample volume is lower than described, please complete the volume with appropriate amount of 1X PBS.
(Compatible) Swab samples	<ol style="list-style-type: none"> Collect swab samples (e.g., eye, nasal, pharyngeal, or other swabs) in liquid transport media or 1 ml PBS containing a common fungicide. Incubate for 30 minutes at room temperature. Dispense 100-560 μl (EVO 100-400 μl) of sample into each Sample Tube.

*Recommended Kit is the **MagPurix® Viral/Pathogen Nucleic Acids Extraction Kit B (ZP02012)**

Note:

Plasma must be prepared from fresh or frozen blood samples collected in tubes that contain common anti-coagulants like EDTA and citrate. (Heparin has inhibitory effects on nucleic acid amplification reaction).

RNA Carrier has two roles in the purification process. First, it enhances the binding of viral nucleic acids to the silica surface of magnetic particles, especially when there are few target molecules in the sample. Second, in rare cases that chaotropic salts and detergents in the lysis buffer may not denature RNase, RNA Carrier can help protecting RNA from degradation. If RNA Carrier is not added to the reaction, recovery of DNA or RNA may be reduced.

Using fresh sample (stored at 2-8°C for up to 6 hours) for extraction is recommended. Total nucleic acid yield and quality will decrease with time or after multiple freeze-thaw cycles. For longer storage time, samples should be frozen at -20°C or lower and avoid freeze-thaw cycles. Thaw the samples at room temperature (15-25°C) and process the sample immediately after the temperature reaches to room temperature. **Do not** refreeze sample after thawing. If precipitation is visible in the sample, centrifuge at 6,800 x g for 3 minutes and transfer supernatant to a new tube without disturbing the precipitate, and immediately start the purification procedure.

For large volume liquid samples with low or unknown viral content, e.g., urine or other, follow the “Urine” preparation concentrate procedure.


Table A – The suggested starting material and elution volume range for each nucleic acid extraction		
Sample type	Starting material per sample	Elution Volume
Serum	100-560 µl (EVO 100-400 µl)	50-300 µl (EVO 50-200 µl)
Plasma		
Cerebrospinal fluid (CSF)		
Pretreated urine	100-560 µl (EVO 100-400 µl) *Large volume liquid sample pretreatment	
Cell-free body fluids	100-560 µl (EVO 100-400 µl)	
Swab samples		

Preparation of RNA Carrier

RNA Carrier	<ol style="list-style-type: none"> Gently spin the RNA Carrier tube before opening it. Add 1.0 ml RNase-free water to lyophilized RNA Carrier and mix by vortex. Store RNA Carrier at 4°C (short-term, up to 1 month) or at -20°C (long-term, aliquots before freezing). Avoid freeze-thaw more than 3 times. Before extraction, add 5 µl (for 100 µl sample), 10 µl (for 200 µl sample) or 20 µl (for 400 µl sample) RNA Carrier into each Sample Tube.
-------------	--

Procedure of MagPurix System

Workflow of MagPurix operation

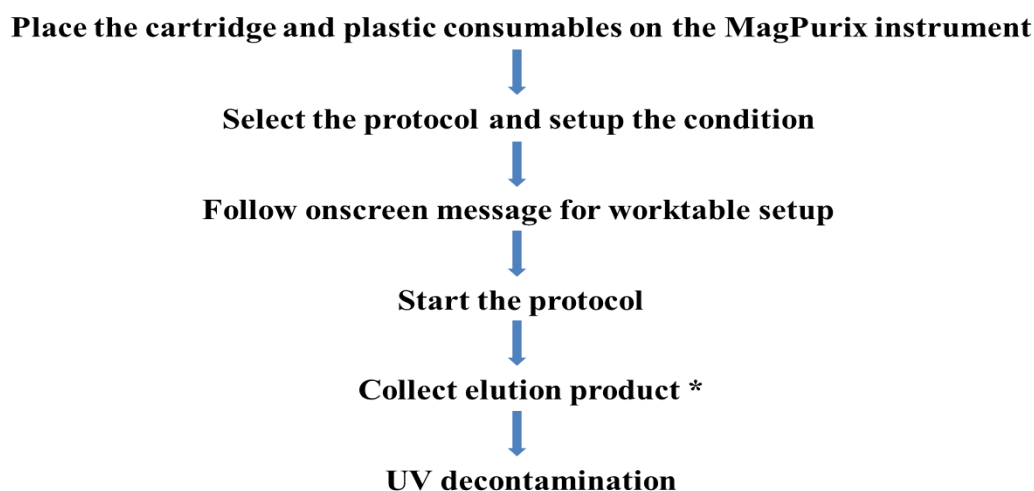

* Output the bench record (option)


Purification Protocol - MagPurix® series


1	Turn on the Instrument	a. Turn on the power switch and wait for the screen to turn on.
2	Load new Consumable(s) and Cartridge(s)	a. Open the door and remove the Sample Rack from the instrument. b. Load 1 Reagent Cartridge, and all plastic disposables (2 Reaction Chamber, 3 Tip Holder, 4 Piercing Pins, 5 Filter Tips and other components presented in the kit intended to use). c. Place 6 Sample Tubes and 7 Elution Tubes into the Sample Rack.
3	Load the Samples	a. Transfer appropriate volume of sample into each Sample Tube on the Sample Rack. b. Put the Sample Rack back into the instrument and close the door.
4	Program Set up	a. Scan the protocol barcodes to select the purification protocol, sample volume and elution volume.
5	Start Extraction	a. Follow the instructions displayed on the screen to double-check the operating steps being completed before program running. b. Press " ENTER " to start the experiment. Instrument will run the protocol program automatically until the whole process is completed. c. At the end of the run (approximately 12 series 40-55 minutes , 24 series 40-70 minutes), instrument alarms briefly.

-
- 6** Collect the Elution Tubes
- Open the instrument door.
 - Collect the Elution Tubes containing the purified nucleic acids.
 - The purified nucleic acids are ready for immediate use. Store the purified nucleic acids at 4°C (short-term, less than 10 days) or aliquot and store at -70°C (long-term) before performing downstream analysis.
 - Discard the used cartridges and all plastic consumables into biohazard waste. ***Do not reuse the cartridges.**
 - If you are not using the instrument immediately, place the Sample Rack back to the workplace, close the instrument door and press “Start” button for 2 seconds to enter sleep mode. If the instrument will not be used in an extended period of time, please turn off the power switch.
-

Purification Protocol - MagPurix® EVO series

-
- 1** Turn on the Instrument
- Turn on the power switch and wait for the screen to turn on
 - Login the instrument and enter the Home Page.
-
- 2** Load new Consumable(s) and Cartridge(s)
- Open the door and remove the Sample Rack from the instrument.
 - Open the Tip-Holder Lid.
 - Load **1** Reagent Cartridge and all plastic disposables (**2** Reaction Chamber, **3** Tip Holder, **4** Piercing Pins, **5** Filter Tips and other components presented in the kit intended to use).
 - Close the Tip-Holder Lid.
 - Paste the Barcode Stickers on the Elution Tubes.
 - Place **6** Sample Tubes and **7** Elution Tubes into the Sample Rack.
-
- 3** Load the Samples
- Transfer appropriate volume of sample into sample tubes on Sample Rack.
 - Put the Sample Rack into the instrument and close the door.
-
- 4** Program Set up
- Select the appropriate protocol program on the instrument. Press **NEXT**.
 - Select the appropriate Sample Volume and Elution Volume and press **NEXT**.
 - Press the number button to select the right Sample Numbers.
 - Scan/Edit each primary Sample ID directly. After finished, press **NEXT**.
 - Scan/Edit each Elution Tube ID directly. After finished, press **NEXT**.
 - Scan Reagent Cartridge Barcode. Press **NEXT**.
 - *If the cartridge is expired, the next step cannot be performed.**
 - Follow the instructions on the screen to double-check the operating steps being completed before running the program. Press **NEXT**.
-
- 5** Start Extraction
- Check “**PROGRAM CONFIRMATION**” on the screen.
 - Press “**START**” to start the experiment. Instrument will run the protocol automatically until the whole process is completed.
 - At the end of the run (approximately **40-50 minutes**) (**RAPID: 19-23 minutes**), instrument alarms briefly and the screen indicates “**PROGRAM FINISH**”.
 - If you want to perform the same protocol, press “**RERUN**” to perform the same experiment. If you do not need to re-run the
-

experiment, press the function button “ HOME” to exit the experiment mode.

- 6** Collect the Elution Tubes
- Open the instrument door.
 - Collect the Elution Tubes containing the purified nucleic acids.
 - The purified nucleic acids are ready for immediate use. Store the purified nucleic acids at 4°C (short-term, less than 10 days) or aliquot and store at -70°C (long-term) before performing downstream analysis.
 - Discard the used cartridges and all plastic consumables into biohazard waste. ***Do not reuse the cartridges.**
 - If you are not using the instrument immediately, please put the Sample Rack back into the instrument, close the instrument door, and press the “ POWER” function button to enter sleep mode. If the instrument will not be used in an extended period of time, please turn off the power switch.

Troubleshooting

***This table is helpful for solving common problem. If you need other technical support, please contact Zinexts team (sales@zinexts.com) or your distributor.**

Problem	Possible Cause	Comments and suggestions
Poor DNA quality or yield	Deterioration or contamination of reagents.	Please ensure that the kit reagents are still within the effective shelf-life period before use. Discard any kit reagent that shows discoloration or evidence of microbial contamination.
	Kit stored under non-optimal conditions.	Store kit at 15-25°C at all time after arrival. If either reagent or buffer precipitate upon shipping in cold weather or during long-term storage, dissolve precipitates by gently warming and stirring the solution. Please do not freeze the Reagent Cartridges.
	Insufficient sample input.	DNA yield depends on the sample type and the number of nucleated cells in the sample. Please proportionally adjust the total input amount of sample to increase the DNA yield.
	Too much of elution buffer was used.	The elution volume can be reduced proportionally.
	The eluate of final product(s) is not enough.	Please collect issue information and provide it to your Support Representative/Technical Support as soon as possible.
Clogging issue	Too much sample material was used.	Decrease the input amount of sample material or dilute your sample.

Problem	Possible Cause	Comments and suggestions
No results in downstream analysis	No signal / The PCR was inhibited.	Using appropriate controls for analysis. Check the positive control, negative control, water (NTC) and internal control to clarify the possible causes.
Instrument malfunction / abnormal sound	Abnormal consumables: 1. Deformed Filter Tips 2. Deformed Reaction Chamber 3. Deformed Tip Holder	Please replace the batch with normal consumables.
	Abnormal action of instrument: 1. Inaccurate correction value 2. Spare parts or components damaged	Please collect issue information (videos and pictures) and provide it to your Support Representative/Technical Support as soon as possible to calibrate or replace any other damaged or worn parts.

Related Products











Product Name	Cat. no.
MagPurix® Blood DNA Extraction Kit 200	ZP02001
MagPurix® Blood DNA Extraction Kit 1200	ZP02002
MagPurix® Viral Nucleic Acid Extraction Kit	ZP02003
MagPurix® Tissue DNA Extraction Kit	ZP02004
MagPurix® Cultured Cell DNA Extraction Kit	ZP02005
MagPurix® Bacterial DNA Extraction Kit	ZP02006
MagPurix® HPV DNA Extraction Kit for Swab Samples	ZP02007
MagPurix® TB DNA Extraction Kit	ZP02008
MagPurix® FFPE DNA Extraction Kit	ZP02009
MagPurix® Forensic DNA Extraction Kit	ZP02010
MagPurix® Viral/Pathogen Nucleic Acids Extraction Kit A	ZP02011
MagPurix® Viral/Pathogen Nucleic Acids Extraction Kit B	ZP02012
MagPurix® Viral RNA Extraction Kit	ZP02013
MagPurix® Plant DNA Extraction Kit	ZP02014
MagPurix® Total RNA Extraction Kit	ZP02015
MagPurix® Viral Nucleic Acid Extraction Kit LV	ZP02016
MagPurix® CFC DNA Extraction Kit	ZP02017
MagPurix® cfDNA Extraction Kit Plus	ZP02024
MagPurix® cfDNA Extraction Kit LV	ZP02025
MagPurix® Coronavirus RNA Extraction Kit	ZP02027
MagPurix® Urine cfDNA Extraction Kit	ZP02032
MagPurix® Plasma cfDNA Extraction Kit	ZP02033

References

- Tan SC *et al.* J Biomed Biotechnol. (2009)

Symbols

The following symbols are used on labels and in Instructions for Use (IFU), in compliance with EN ISO 15223-1 standard.

Symbol	Explanation
	CE mark
	For In Vitro Diagnostic Use
	Catalogue number
	Lot/Batch number
	Sufficient for [n] samples
	Expiry date
	Storage temperature (15°C - 25°C)
	Manufacturer
	European Authorized Representative
	Caution

Limited Product Warranty

Zinexts Life Science is committed to provide customers with high-quality products and services. Our goal is to ensure that every customer is 100 % satisfied with our products and services. If you have any question or concerns, contact our Technical Support Representatives.

Zinexts Life Science guarantees the performance of all products according to the specifications stated in our product literature. The purchasers/users must determine the suitability of the product for their particular use. We reserve the right to change, alter, or modify any product to enhance its performance and design.

This warranty limits Zinexts Life Science Corporation's liability only to the cost of the product. No warranty is granted for products beyond their listed expiration date. No warranty is applicable unless all product components are stored and used in accordance with instructions.

Revision History

Version	Date	Description
2.2	13. Apr. 2023	<ol style="list-style-type: none">1. Correct typo and format2. Related products: add ZP02032 and ZP02033